

FIG. 1

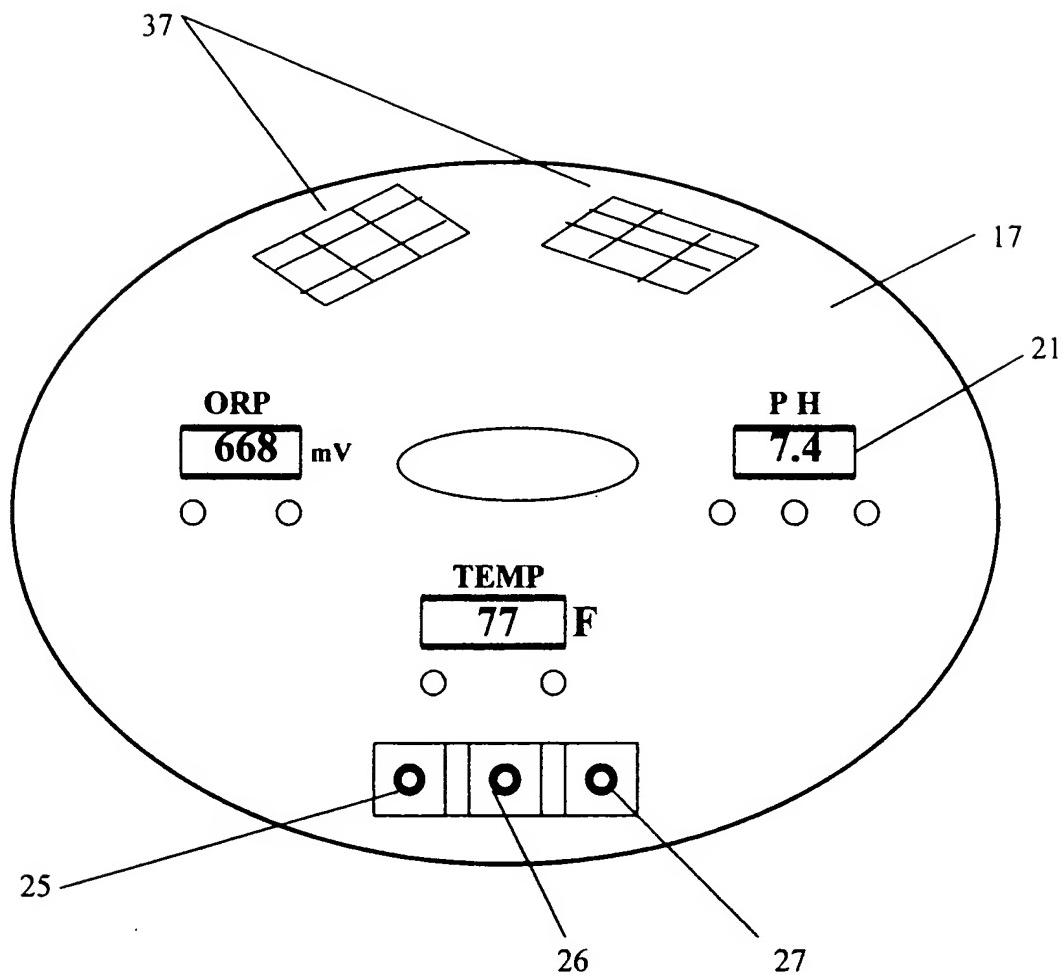


FIG. 2

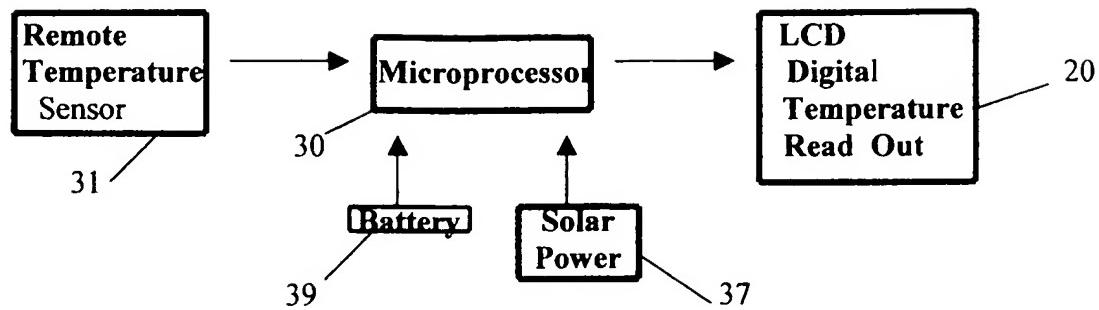


FIG. 3

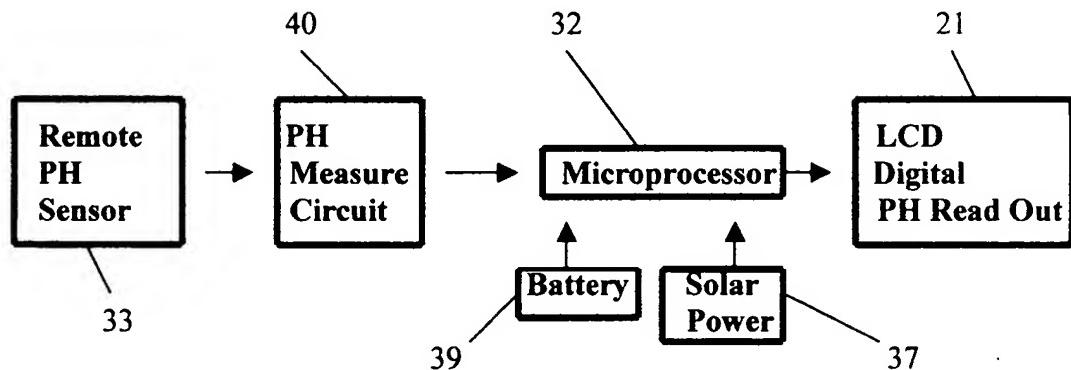


FIG. 4

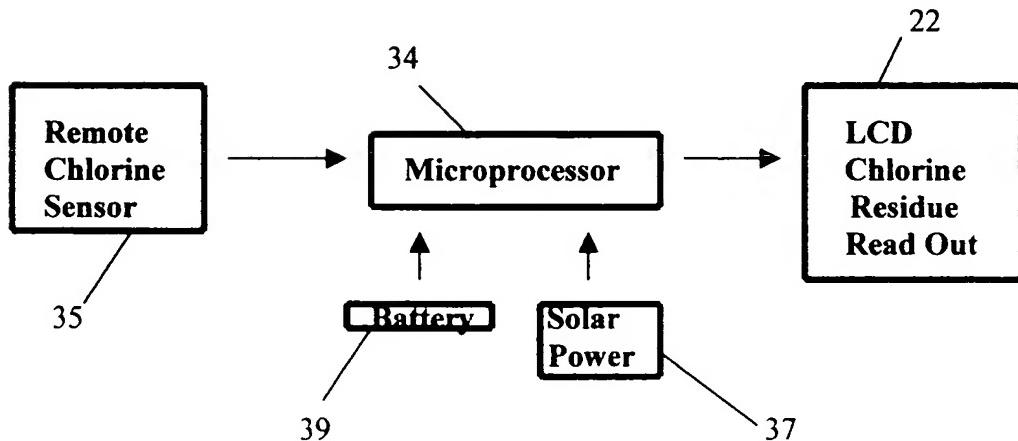


FIG. 5

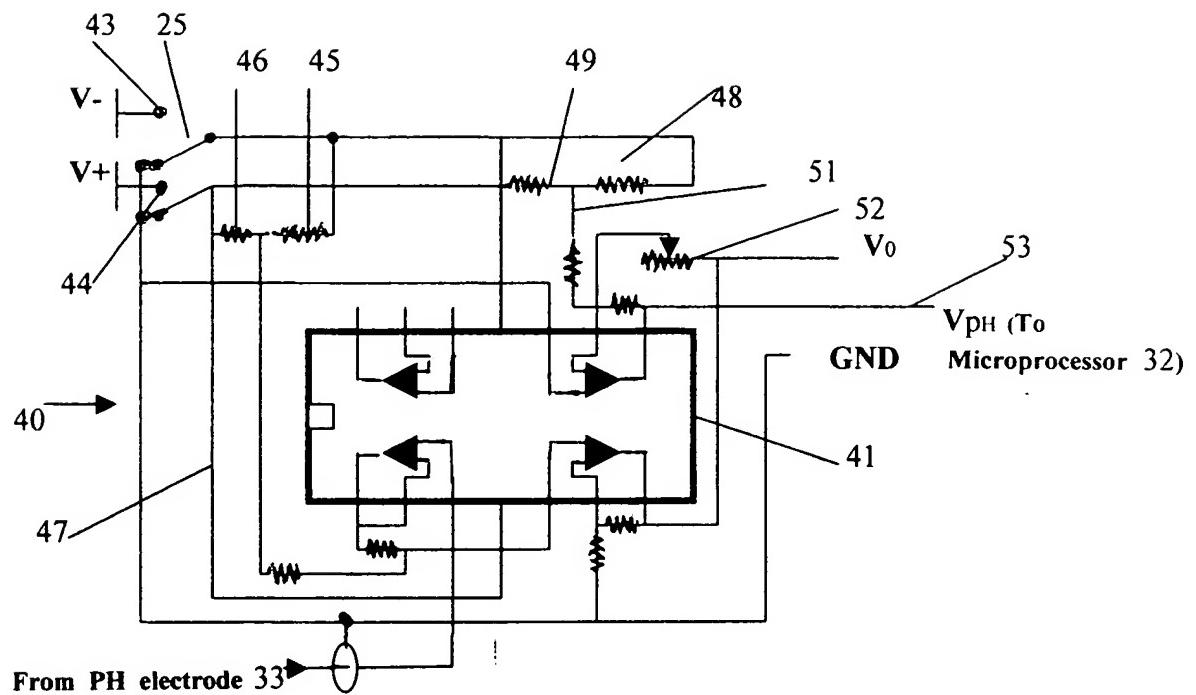


FIG. 6



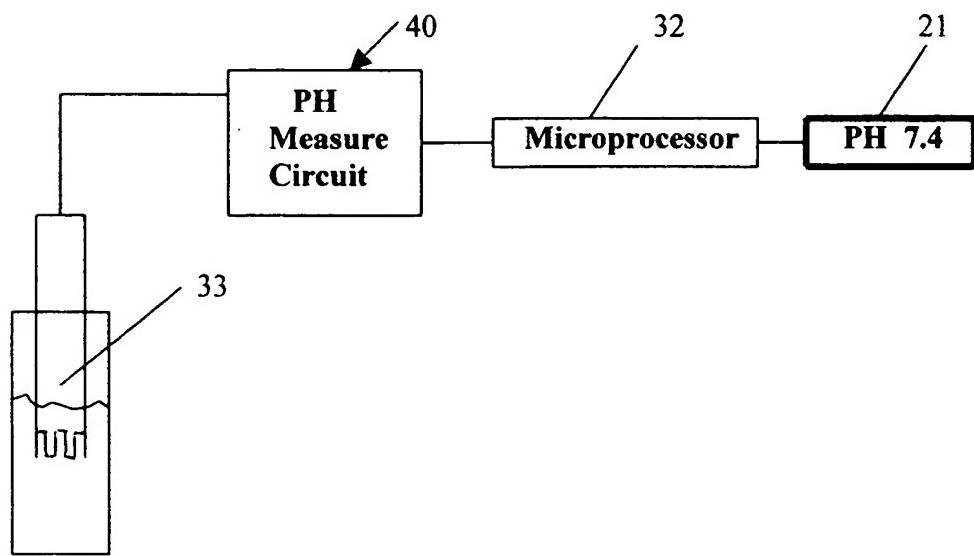


FIG. 7

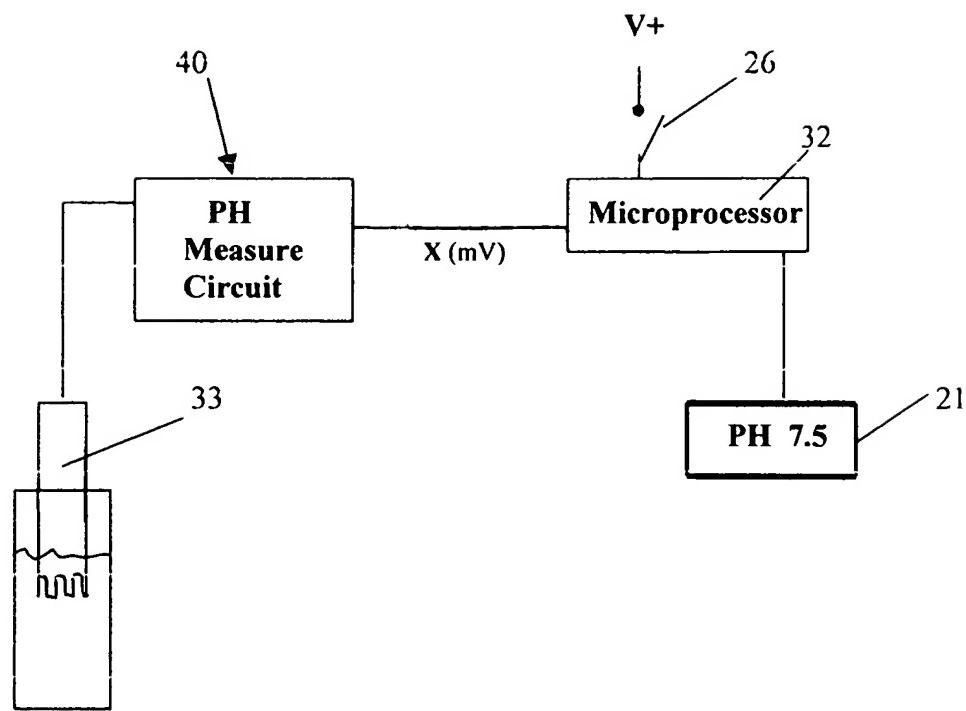

PH 7.50 Buffer

FIG. 8

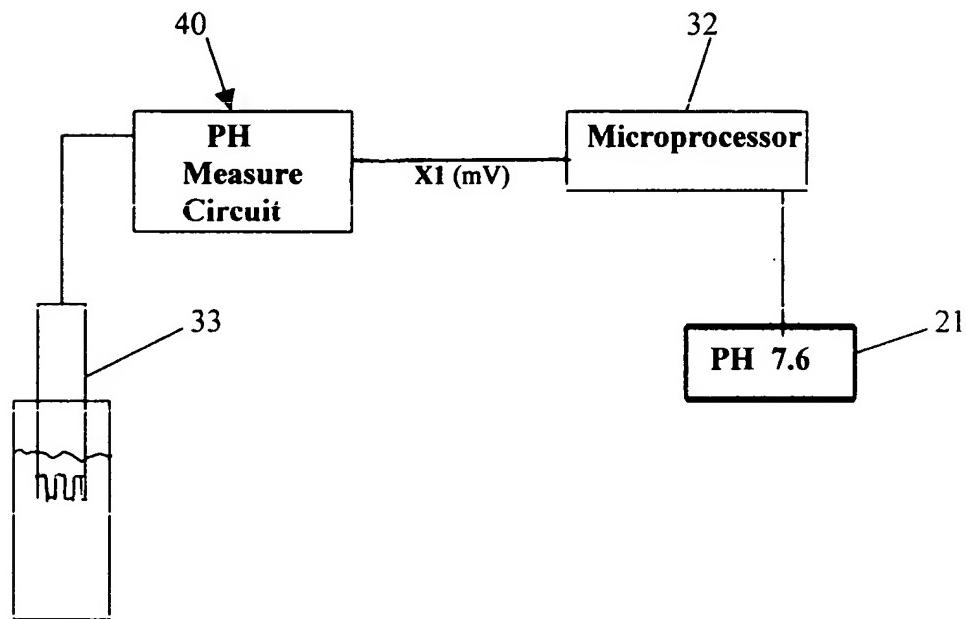

PH 7.6 Water Sample

FIG. 9